



# AriaII 5G 3R 2B 2V 2UV

Cytometer:	FACSAriaII	User:	Christiane
Cytometer Name:	FACSAriaII	Institution:	
Serial Number:	P46900021	Software:	BD FACSDiva 6.1.1
Input Device:	Manual	Date:	6/27/2012 9:10:11 AM
Sheath Pressure:	12.00		
Nozzle Size:	130		
Window Extension:	2.00		


Blue Laser  
(488nm)  
FSC

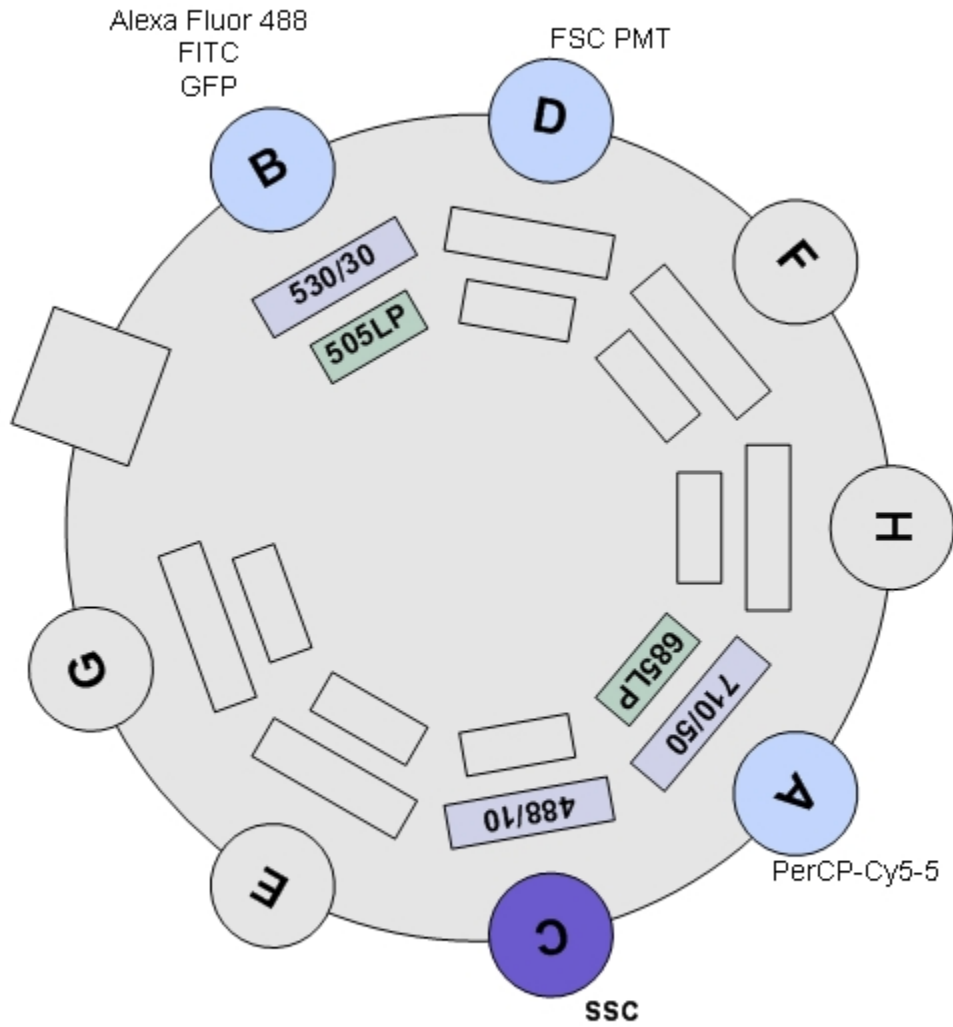


Violet Laser  
(405nm)

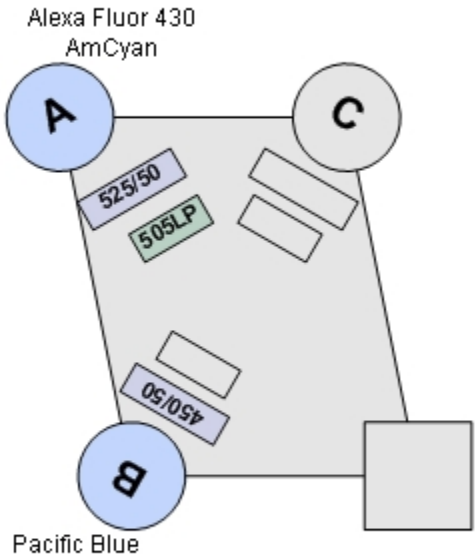


355 UV Laser  
(355nm)

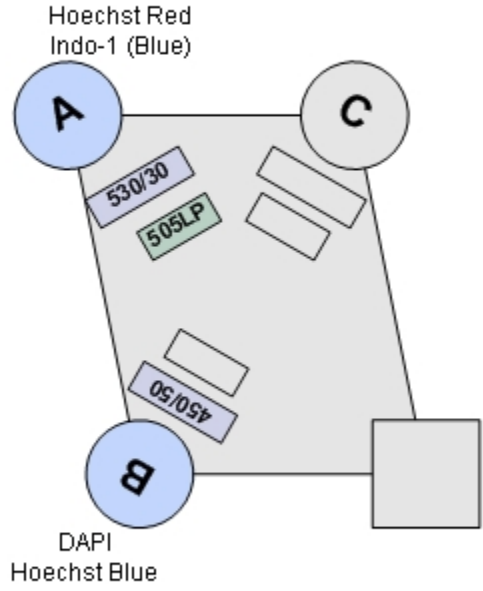

Red Laser  
(633nm)

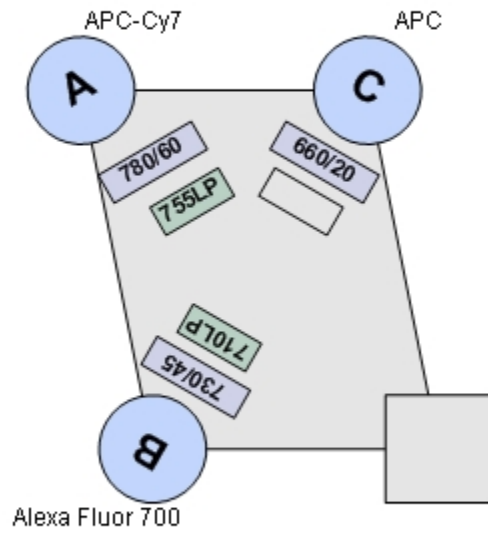

YELLOW/GREEN Laser  
(561nm)

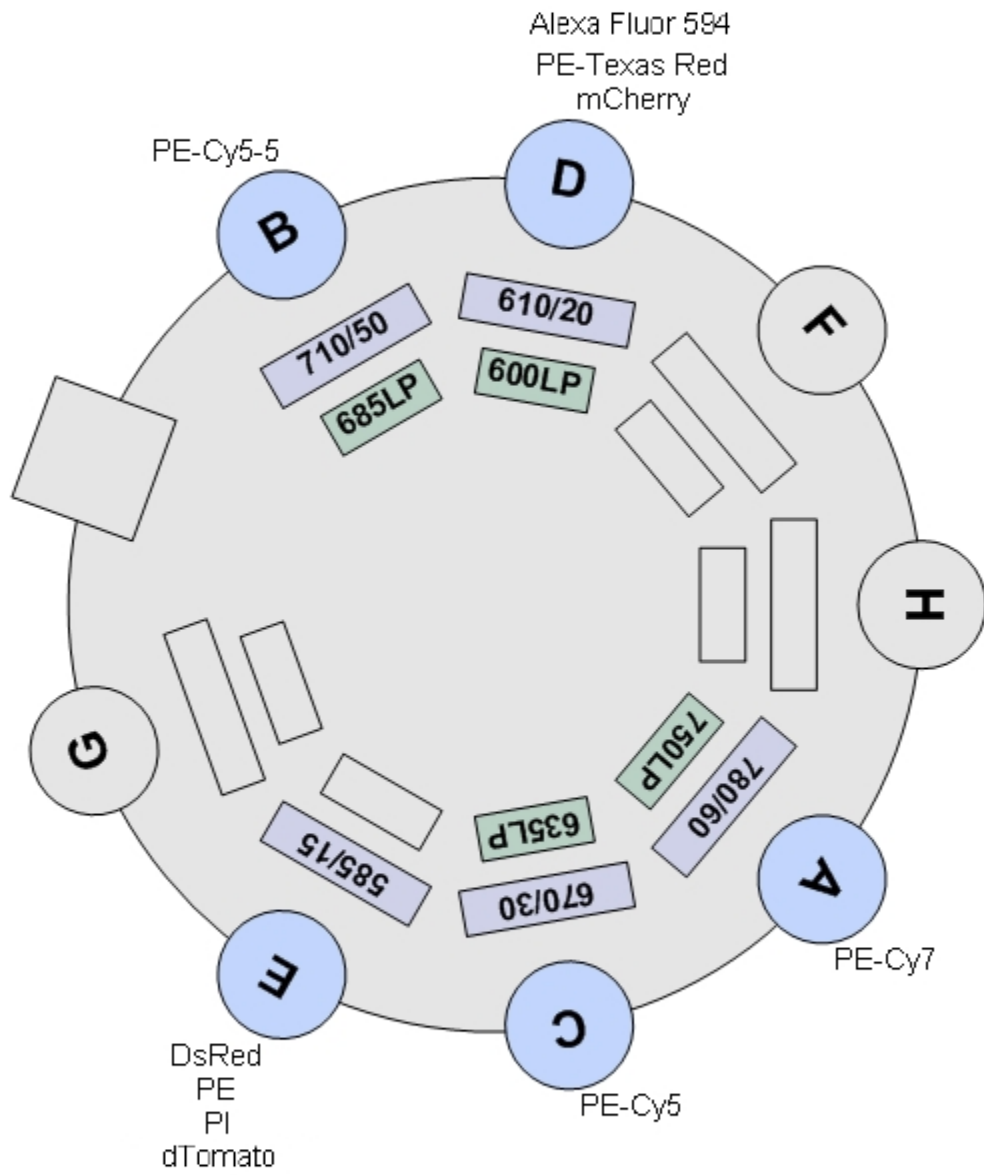

Comments: